
This is an electronic reprint of the original article.
This reprint may differ from the original in pagination and typographic detail.

Maham, Kinza; Vaskuri, Anna; Manoocheri, Farshid; Ikonen, Erkki
Calibration of Near-Infrared Detectors Using a Wavelength Tunable Light Source

Published in:
OPTICAL REVIEW

DOI:
[10.1007/s10043-020-00586-9](https://doi.org/10.1007/s10043-020-00586-9)

Published: 01/04/2020

Document Version
Publisher's PDF, also known as Version of record

Published under the following license:
CC BY

Please cite the original version:
Maham, K., Vaskuri, A., Manoocheri, F., & Ikonen, E. (2020). Calibration of Near-Infrared Detectors Using a Wavelength Tunable Light Source. *OPTICAL REVIEW*, 27(2), 183-189. <https://doi.org/10.1007/s10043-020-00586-9>

This material is protected by copyright and other intellectual property rights, and duplication or sale of all or part of any of the repository collections is not permitted, except that material may be duplicated by you for your research use or educational purposes in electronic or print form. You must obtain permission for any other use. Electronic or print copies may not be offered, whether for sale or otherwise to anyone who is not an authorised user.



The 13th Japan-Finland Joint Symposium on Optics in Engineering (OIE'19), Espoo, Finland and Tallinn, Estonia

Calibration of Near-Infrared Detectors Using a Wavelength Tunable Light Source

Kinza Maham¹ · Anna Vaskuri^{1,3} · Farshid Manoocheri¹ · Erkki Ikonen^{1,2}

Received: 15 October 2019 / Accepted: 1 February 2020
© The Author(s) 2020

Abstract

This paper presents the spectral responsivity calibrations of two indium gallium arsenide (InGaAs) and one germanium based near-infrared photovoltaic detectors using a wavelength tunable laser source based on a supercontinuum laser developed at the Metrology Research Institute, Aalto University. The setup consists of a supercontinuum laser based on a photonic crystal fiber as the light source, a laser line tunable filter, and coupling optics. These responsivity calibrations are performed against a pyroelectric radiometer over a wide spectral range of 800–2000 nm. Our wavelength tunable laser source has a high spectral power up to 2.5 mW with a narrow spectral full-width-at-half-maximum of 3 nm at a wavelength of 1100 nm. Despite the sharp spectral intensity variations, no artifacts are observed in the spectral responsivities of the detectors. Comparison of the spectral responsivities of the InGaAs detectors measured using the wavelength tunable laser and the earlier calibrations performed at the Metrology Research Institute in 2010 and 2016, shows that the higher spectral power of wavelength tunable light source decreases the expanded uncertainty from approximately 4% to 2.2–2.6% over the spectral range of 820–1600 nm. Temperature dependence of the spectral responsivities near the band gap edges are also measured and analysed.

Keywords Near-infrared detectors · Spectral responsivity · Supercontinuum laser · InGaAs · Ge

1 Introduction

Absolute calibration of optical detectors is important for the reliability of optical characterization methods and, therefore, has significant applications in optics and metrology. Absolute cryogenic radiometer (ACR), based on electrical substitution, has been used as a primary standard instrument in optical power calibrations of detectors at many metrology institutes since 1980's [1–3]. However, when ACRs are coupled with traditional lamp-monochromators, limited radiant flux of about 100 nW/nm is observed even at moderate spectral resolution, as the lamp-monochromator systems

have finite etendue [4]. To address this shortcoming, several wavelength tunable laser source setups based on dye, Ti:Sapphire, or supercontinuum laser have been explored mainly in the visible range [5–12].

Supercontinuum (SC) laser is a source of broad, coherent, and continuous wave white light emission over the broad spectral range from 350 to 2500 nm. SC lasers are based on a photonic crystal fiber (PCF) with a range of available pump powers. These lasers also have three orders of magnitude higher radiant flux of 5 mW/nm in comparison to typical lamp-monochromators [4]. Therefore, SC lasers can be employed in many fields including optical metrology as they allow measurements with low etendue, high power, and high spectral resolution.

In this paper, we present a newly developed monochromatic light source based on a SC laser for the spectral responsivity calibrations of two indium gallium arsenide (InGaAs) and one germanium (Ge) based photovoltaic near-infrared detectors at the spectral range of 800 nm–2000 nm. A laser line tunable filter (LLTF) is used to obtain a collimated wavelength tunable light beam from

✉ Kinza Maham
kinza.maham@aalto.fi

¹ Metrology Research Institute, Aalto University, P.O. Box 15500, FI-00076 Aalto, Finland

² VTT MIKES, P.O. Box 1000, FI-02044 VTT Espoo, Finland

³ Present Address: National Institute of Standards and Technology, Boulder, CO, USA

the supercontinuum laser. These spectral responsivity calibrations are performed against a calibrated pyroelectric radiometer which has a spectrally flat responsivity.

The setup introduced in this paper is automated using custom-made LabVIEW software, which increases the detector alignment accuracy and repeatability of the calibration measurements. Furthermore, our wavelength tunable laser source developed provides narrower spectral bandwidths with higher optical power output compared to traditional lamp-based monochromators. Effects of sharp spectral features in the source spectrum are analysed and found to be insignificant. Our setup decreases the expanded uncertainty in the spectral responsivity calibrations to approximately 2.3%.

2 Optical setup and measurement sequence

The optical setup of the wavelength tunable laser source developed for the spectral responsivity calibrations of the photovoltaic detectors is presented in Fig. 1. A supercontinuum laser based on PCF is the source of optical radiation in our setup. The low etendue of the supercontinuum laser enables accurate collimation. We have used a laser line tunable filter (LLTF) in order to obtain wavelength tunable light beam from the supercontinuum laser. LLTF is based on volume holographic Bragg grating made of silver halide glass, which is a non-hygroscopic material and is transparent between 400 and 2500 nm. The input beam is diffracted by the gratings present in the LLTF. Figure 2 shows a simplified design of the LLTF.

In order to select the diffracted wavelength of light, the angle of the grating is adjusted to meet the Bragg's condition $\lambda_b = 2n_o \Lambda \cos(\Theta + \phi)$, where λ_b is the Bragg wavelength, Λ is the period of the grating, n_o is the refractive index of the photo-thermo-refractive glass, Θ is the angle between incident light and normal of the grating surface, and ϕ is the inclination of Bragg plane which is defined as the angle between the normal of the grating surface and the grating vector [14]. If the light beam does not satisfy the Bragg condition, it passes through undiffracted. Only a particular narrow wavelength range fulfills Bragg condition and

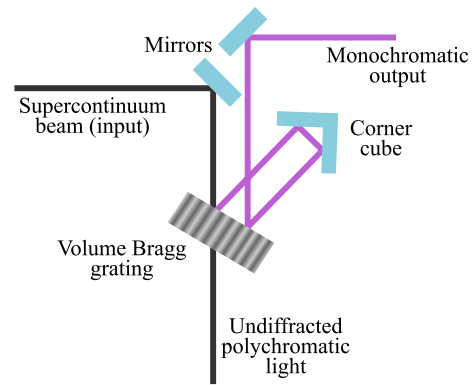


Fig. 2 Design of the laser line tuneable filter (LLTF) based on a volume Bragg grating. The figure is modified from [13]

interferes constructively with the refractive index modulation. The diffracted light is reflected on a second region of the Bragg grating by a corner cube to achieve double diffracted monochromatic output beam.

The LLTF in use consists of two gratings: grating #1 is dedicated to 1000–1700 nm, while grating #2 is dedicated to 1700–2000 nm [15]. The wavelength scale of the LLTF is characterized using a scanning spectroradiometer and wavelength shifts as presented in Table 1, are observed and corrected from the final spectral responsivity calibration results.

The standard uncertainty of $\Delta\lambda$ is estimated by deviations from a smooth fitting curve and it also includes the uncertainty contribution from the calibration of the spectroradiometer. A standard uncertainty of 0.03% is present in the spectral responsivities of the photovoltaic detectors due to the wavelength of the laser after correction.

The spectroradiometer used for the characterization of LLTF is calibrated using mercury (Hg) and argon (Ar) calibration pen lamps. These calibration lamps produce intense fundamental spectral lines from the excitation of Hg vapor and Ar that do not shift with the temperature and time.

The collimated light from LLTF is coupled into a multimode fiber having a numerical aperture (NA) of 0.22. To ensure optimal coupling of the beam into the fiber, a lens is placed in the fiberoptic module connected at the output port of the LLTF. The multimode fiber terminates into a

Fig. 1 Wavelength tunable filter light source setup, based on a supercontinuum laser and a laser line tunable filter (LLTF) used for measuring the spectral responsivity of photovoltaic detectors

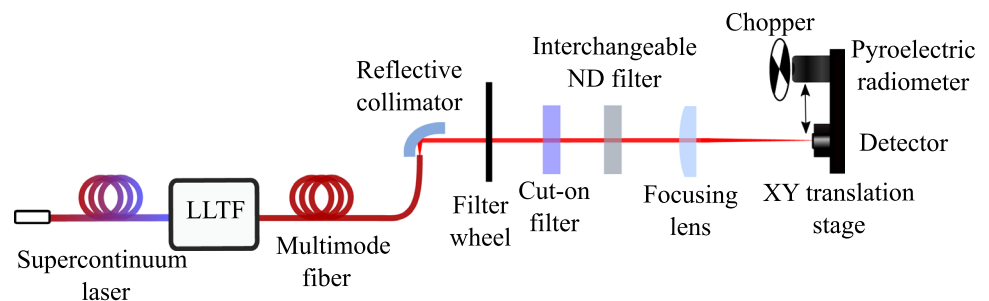


Table 1 Wavelength shift $\Delta\lambda$ between the observed wavelength and the set wavelength of the LLTF with its standard uncertainty


Observed λ/nm	Set λ/nm	$\Delta\lambda/\text{nm}$	Standard uncertainty/ nm
997.06	1000	-2.94	0.15
1097.33	1100	-2.67	0.15
1197.15	1200	-2.85	0.15
1297.22	1300	-2.78	0.15
1397.23	1400	-2.77	0.15
1497.37	1500	-2.63	0.15
1597.66	1600	-2.34	0.15
1702.23	1700	2.23	0.25
1801.19	1800	1.19	0.25
1900.74	1900	0.74	0.25
1999.28	2000	-0.72	0.25

reflective collimator, based on a 90° off-axis parabolic mirror. A motorized filter wheel, controlled by LabVIEW software, is used to measure dark and signal voltages for each wavelength [16]. We observed that the LLTF produces strong second and third harmonics in the visible wavelength range. Therefore, a cut-on filter with up to 99.9% attenuation of all the wavelengths below 800 nm was used for filtering the harmonics.

The laser setup has an average power of up to 0.3 mW within a 3 nm band from 800–2000 nm. In order to avoid saturation of the detectors, an interchangeable neutral density filter with the optical density of 0.5 is used to attenuate the optical power of the beam. The setup produces a collimated uniform beam with a narrow diameter of approximately 2 mm. The setup is further automated by mounting the photovoltaic and reference detectors on a high-resolution XY translation stage, which allows us to obtain the pyroelectric reference signal and detector voltage signal with high precision for every wavelength.

The pyroelectric radiometer is a thermal detector, with a lithium tantalate pyroelectric probe, which operates on the principle of temperature change induced temporal voltage difference [17, 18]. We use it as a reference detector because it has a flat spectral responsivity. Our pyroelectric radiometer runs at a chopping frequency of 30 Hz. The reference detector is calibrated against a silicon trap detector at a wavelength of 647 nm. The calibration of the pyroelectric radiometer and its spectral flatness accounts for a standard uncertainty of 1%.

The spectral responsivities of detectors are measured from 800–2000 nm with an interval of 0.5 nm. A delay of 50 ms is added before each reading, to ensure the detectors have stabilized. A current-to-voltage converter is used with the photovoltaic detectors. The measurement sequence of the software records four sets of voltages for each wavelength:

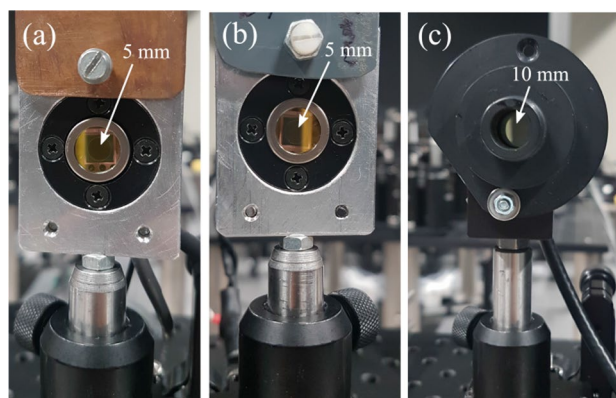**Fig. 3** Detectors studied in this work: InGaAs #1 detector with an aperture of 5 mm (a), InGaAs #2 with an aperture of 5 mm (b), and Ge detector with an aperture of 10 mm (c)

reference signal voltage $V_{p, \text{signal}}$, dark reference voltage $V_{p, \text{dark}}$, signal voltage of the detector V_{signal} and dark voltage of the detector V_{dark} . For each wavelength between 800 and 2000 nm in the calibration, the spectral responsivity (A/W) is calculated as

$$R = \frac{I}{P_{\text{ref}}}, \quad (1)$$

where I is measured photocurrent generated by the photovoltaic detector under test and P_{ref} is the reference power of pyroelectric radiometer. Current of the photodetectors is calculated from the measured voltages as, $I = (V_{\text{signal}} - V_{\text{dark}}) \cdot \frac{1}{G_{\text{CVC}}}$, where G_{CVC} is the calibrated gain of a current-to-voltage converter (CVC). In order to calculate the reference power, equation $P_{\text{ref}} = c_p \cdot (V_{p, \text{signal}} - V_{p, \text{dark}})$ is used, where the correction factor c_p includes the correction from the absolute calibration of the pyroelectric radiometer.

3 Results

Figure 3 is a photograph of the InGaAs #1, InGaAs #2, and Ge photovoltaic detectors calibrated against a pyroelectric radiometer. These detectors have wavelength dependent spectral responsivities, fast response times, and high sensitivities [19].

The InGaAs detectors shown in Fig. 3 have an aperture diameter of 5 mm and operate over the spectral range of 900–1680 nm, with a band gap edge near 1750 nm. The Ge photovoltaic detector has an aperture diameter of 10 mm. It has a high spectral responsivity over a spectral range of approximately 750–1850 nm with a band gap edge at approximately 1650 nm. In this work, we have defined the

usable spectral range as a region where the spectral responsivity exceeds 10% from the maximum response.

3.1 Spectral responsivities of InGaAs detectors

The spectral responsivity calibrations of InGaAs detectors were performed at three different temperatures of 273.15 K, 283.15 K, and 297.15 K. Figures 4a and 5a show the spectral responsivities of InGaAs #1 and InGaAs #2 detectors over the spectral range of 800–2000 nm. The detectors were cooled down with their internal temperature controllers. The incident optical power measured using the pyroelectric radiometer is also shown as the black dotted curve.

As can be seen in Figs. 4a and 5a, the beam power of the wavelength tunable laser varies significantly across the spectral range with a maximum power of approximately 0.7 mW at 1100 nm when the neutral density filter is used. Despite the sharp peaks and irregularities in the spectrum of the supercontinuum laser, no significant deviations are present in the spectral responsivities. To study this, first-order

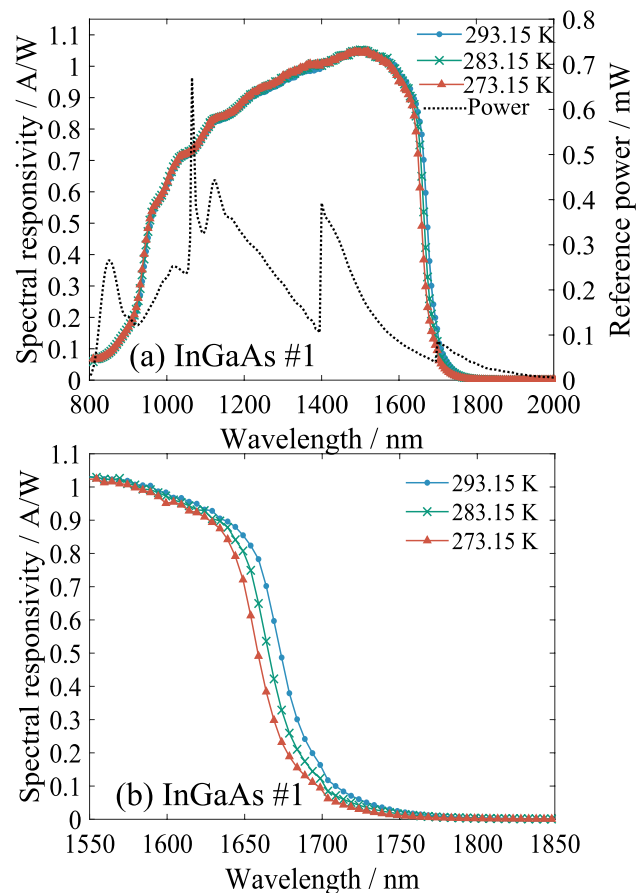


Fig. 4 Spectral responsivity of the InGaAs #1 measured with the wavelength tunable laser source over the spectral range of 800–2000 nm along with the optical reference power (a). Close-up of spectral responsivity of InGaAs #1 near the band gap edge (b)

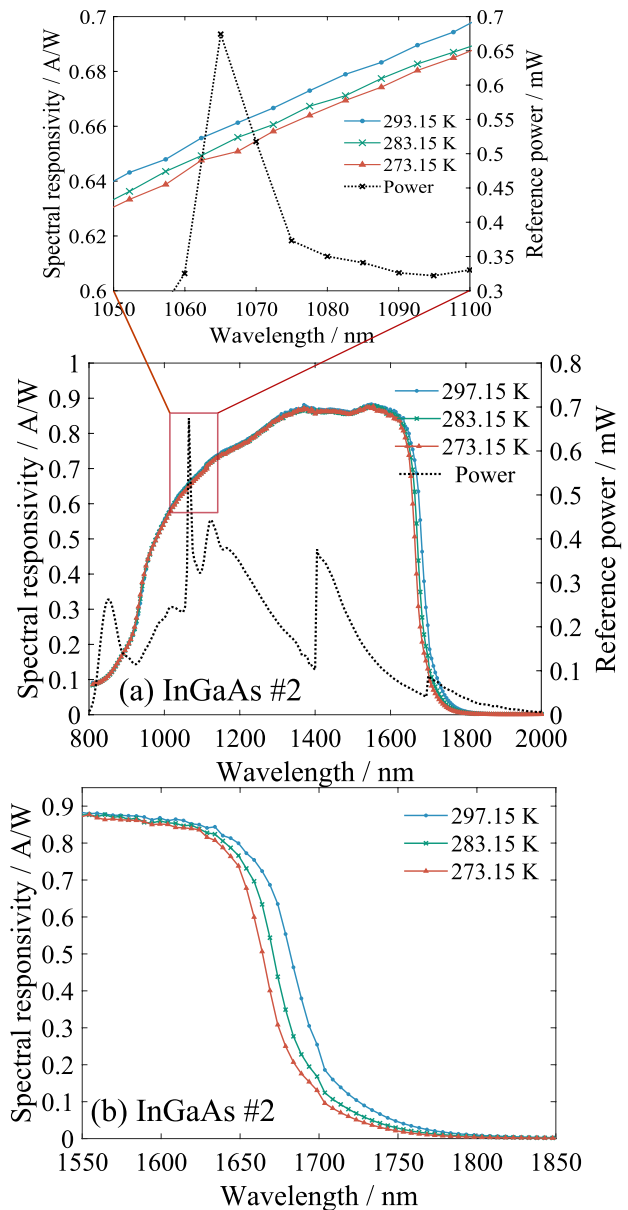


Fig. 5 Spectral responsivity of the InGaAs #2 measured with the wavelength tunable laser source over the spectral range of 800–2000 nm along with the optical reference power (a). Details of the responsivity are magnified close to the peak power. Close-up of spectral responsivity of InGaAs #2 near the band gap edge (b)

polynomials were fitted to the spectral responsivities of InGaAs #2 between 1050 and 1100 nm, close to the peak power. The fitting residuals have relative standard deviations smaller than 0.10%.

The two InGaAs detectors have similar spectral responsivity curves, however, higher oscillations are observed in the spectral responsivity of detector #1. The junction temperature is also an important factor for these detectors since the band gap edge of the spectral responsivity shifts towards shorter wavelengths with decreasing temperature. Figures 4b

and 5b show close-ups of the spectral responsivities of the InGaAs detectors near the band gap edge.

The spectral responsivity calibrations obtained in this work were compared to the older calibrations measured with a reference spectrometer at the Metrology Research Institute, Aalto University [20]. The calibration of InGaAs #1 against the pyroelectric radiometer was compared with the previous calibration performed in 2016 at 283.15 K with an expanded uncertainty of 4%. The comparison plot of InGaAs #1 is presented in Fig. 6a. The spectral responsivity of InGaAs #2 was calibrated in 2010 at the room temperature of 297.65 K \pm 1.5 K with an expanded uncertainty of 4%. The spectral responsivity of InGaAs #2 calibrated in 2010 is presented in Fig. 6b along with the responsivities measured with the wavelength tunable laser source, against a pyroelectric radiometer.

Detector calibrations against the pyroelectric radiometer have an expanded uncertainty of 2.2–2.6% over the spectral range of 820 and 1600 nm depending on the wavelength. The slight difference in our calibration and older reference calibration can be attributed to the uncertainty present in both calibrations. The ageing of the detectors can also be one reason for the different spectral responsivities of InGaAs detectors.

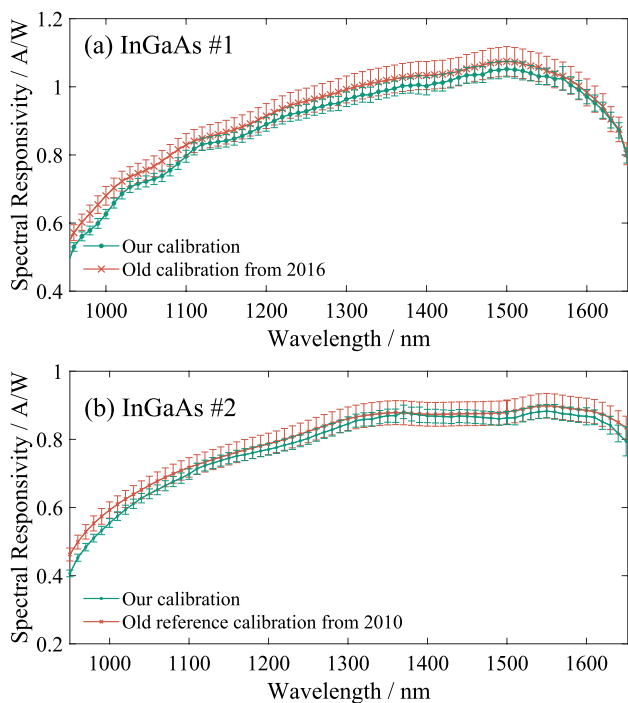


Fig. 6 Comparison of spectral responsivities measured with the wavelength tunable laser source and the reference pyroelectric radiometer with older calibration of InGaAs detectors #1 (a) and #2 (b). The uncertainty bars indicate expanded uncertainties ($k = 2$) in the spectral responsivities

3.2 Spectral responsivity of a Ge detector

Figure 7 shows the spectral responsivity of the Ge detector and reference power recorded using the pyroelectric radiometer.

Unlike InGaAs, this Ge detector does not have a cooling option; therefore, it was calibrated at room temperature that was 298.15 K during the measurements. The Ge detector has low shunt resistance and in turn significant dark current, which highly depends on the temperature, hence, it is very sensitive to the ambient temperature [21]. The Ge photodiode also has an ageing rate of approximately 0.5% per year within a spectral range of 1100 nm–1800 nm as studied by Stock [22] and Lamminpää et al. [23].

3.3 Uncertainty budget

Table 2 gives the uncertainty budget of the detector responsivity calibrations. The pyroelectric radiometer has been calibrated against a calibrated silicon trap detector. The calibration of the pyroelectric radiometer and its spectral flatness accounts for a standard uncertainty of 1%. The uncertainty due to spatial uniformity of the pyroelectric detector is also included in the reference detector uncertainty. The external chopper used with the pyroelectric radiometer produces a standard uncertainty of 0.42% due to the manual adjustment of its phase.

A standard uncertainty of 0.13% is present in the setup due to the alignment of detectors. This uncertainty is determined by tilting the detector by $\pm 1^\circ$ and measuring the relative changes in the detected response. The wavelength of the laser contributes with a standard uncertainty of 0.03%. The spatial nonuniformity of the interchangeable attenuating neutral density filter also contributes with an

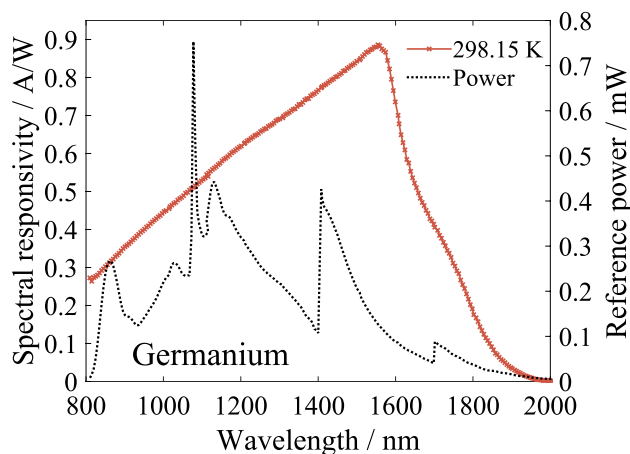
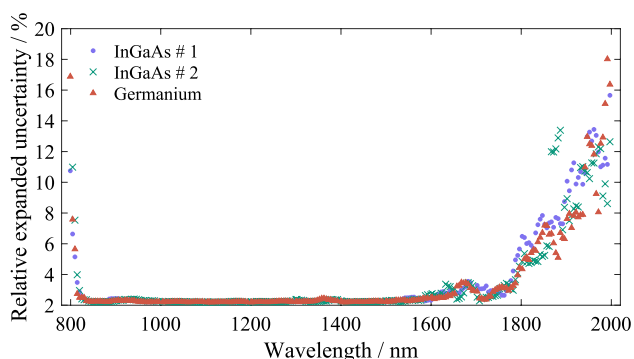


Fig. 7 Spectral responsivity of the Ge detector measured with the wavelength tunable laser source at room temperature along with the reference optical power measured using a pyroelectric radiometer

Table 2 Uncertainty budget of the spectral responsivity of detectors at the wavelength range from 820 to 1600 nm

Source of uncertainty	Uncertainty/%
Reference detector	1.00
Phase resolution of chopper	0.42
Alignment of detector	0.13
Wavelength of laser	0.03
Spatial uniformity of neutral density filter	0.27
Average repeatability of measurement	0.26
Calibration of the current-to-voltage converter	0.001
Calibration of the multimeter	0.001
Combined standard uncertainty ($k = 1$)	1.15
Expanded uncertainty ($k = 2$)	2.30

The pyroelectric radiometer was used as a reference detector

**Fig. 8** Relative expanded uncertainties in the spectral responsivities of the detectors studied from 800–2000 nm

additional standard uncertainty of 0.27%. Another source of uncertainty is the repeatability of the results. The spectral responsivity measurements were repeated three times for every wavelength, and their average and standard deviation were calculated for each wavelength. The average uncertainty calculated due to the repetition of measurements over the spectral range of 820–1600 nm is 0.26%.

Expanded uncertainties for the three detectors are shown in Fig. 8. InGaAs detectors have high spectral responsivity over the spectral range of 900 nm–1680 nm while the Ge detectors have high spectral responsivity between 850–1650 nm. It can also be observed from Figs. 4, 5, and 7, that the signal power of wavelength tunable laser source is high only between 820–1600 nm. Therefore, the expanded uncertainty at these wavelengths is relatively low and starts increasing near at the band gap edges of the detectors. In addition, although our reference pyroelectric radiometer response is supposed to be linear with optical power, we noticed that it behaves nonlinearly below 20 μW . The non-linearity error is 1.7% at 10 μW level and 6.1% at 5 μW level. In practice, this effect increases the spectral responsivity

uncertainties at the spectral range of 1800–2000 nm, where the reference power decreases below 20 μW (Fig. 3a). The spectral range of 800–1800 nm is unaffected by this effect. In these spectral responsivity calibrations, the reference detector causes the highest uncertainty. The expected uncertainty ($k = 2$) can be reduced to 0.5% by using a different reference detector with low uncertainty.

4 Summary

Two InGaAs and one Ge photovoltaic detectors were calibrated using a portable wavelength tunable light source based on a supercontinuum laser. The setup comprises of a supercontinuum laser as a light source, LLTF, and coupling optics. The setup operates over a spectral range of 800–2000 nm with a maximum power of approximately 0.7 mW and full-width-at-half-maximum of 3 nm at a wavelength of 1100 nm. A calibrated pyroelectric radiometer is used as a reference detector due to its flat spectral responsivity.

The spectral responsivities measured were compared to the older calibrations performed in 2010 and 2016, at the Metrology Research Institute, Aalto University. With new setup the expanded uncertainties in the spectral responsivity calibrations decreased from approximately 4% to 2.2–2.6%, at the spectral range of 820–1600 nm. Expanded uncertainties became higher, up to 18%, below 820 nm and above 1600 nm due to the decreasing incident laser power and decreased responsivity near the band gap edges of the photodetectors.

Acknowledgements Open access funding provided by Aalto University.

Open Access This article is licensed under a Creative Commons Attribution 4.0 International License, which permits use, sharing, adaptation, distribution and reproduction in any medium or format, as long as you give appropriate credit to the original author(s) and the source, provide a link to the Creative Commons licence, and indicate if changes were made. The images or other third party material in this article are included in the article's Creative Commons licence, unless indicated otherwise in a credit line to the material. If material is not included in the article's Creative Commons licence and your intended use is not permitted by statutory regulation or exceeds the permitted use, you will need to obtain permission directly from the copyright holder. To view a copy of this licence, visit <http://creativecommons.org/licenses/by/4.0/>.

References

1. Martin, J.E., Fox, N.P., Key, P.J.: A cryogenic radiometer for absolute radiometric measurements. *Metrologia* **21**, 147–155 (1985)
2. Varpula, T., Seppä, H., Saari, J.M.: Optical power calibrator based on a stabilized green He-Ne laser and a cryogenic absolute radiometer. *IEEE Trans. Instrum. Meas.* **38**, 558–564 (1989)
3. Foukal, P.V., Hoyt, C., Kochling, H., Miller, P.: Cryogenic absolute radiometers as laboratory irradiance standards, remote

- sensing detectors, and pyroheliometer. *Appl. Opt.* **29**, 988–993 (1990)
4. Woodward, J.T., Smith, A.W., Jenkins, C.A., Lin, C., Brown, S.W., Lykke, K.R.: Supercontinuum sources for metrology. *Metrologia* **46**, S277–S282 (2009)
 5. Anderson, V.E., Fox, N.P., Nettleton, D.H.: Highly stable, monochromatic and tunable optical radiation source and its application to high accuracy spectrophotometry. *Appl. Opt.* **31**, 536–545 (1992)
 6. Noorma, M., Toivanen, P., Manoocheri, F., Ikonen, E.: Characterization of filter radiometers with a wavelength-tunable laser source. *Metrologia* **40**, S220–S223 (2003)
 7. Ahtee, V., Brown, S.W., Larason, T.C., Lykke, K.R., Ikonen, E., Noorma, M.: Comparison of absolute spectral irradiance responsivity measurement techniques using wavelength-tunable lasers. *Appl. Opt.* **46**, 4228–4236 (2007)
 8. Zarobila, C.J., Patrick, H.J.: Supercontinuum fiber laser source for reflectance calibrations in remote sensing. *Proc. SPIE* **7807**, B-1–16 (2010)
 9. Ceolato, R., Riviere, N., Hespel, L.: Reflectances from a supercontinuum laser-based instrument: hyperspectral, polarimetric and angular measurements. *Opt. Express* **20**, 29413–29425 (2012)
 10. Schuster, M., Nevas, S., Sperling, A., Völker, S.: Spectral calibration of radiometric detectors using tunable laser sources. *Appl. Opt.* **51**, 1950–1961 (2012)
 11. Levick, A.P., Greenwell, C.L., Ireland, J., Woolliams, E.R., Goodman, T.M., Bialek, A., Fox, N.P.: Spectral radiance source based on supercontinuum laser and wavelength tunable bandpass filter: the spectrally tunable absolute irradiance and radiance source. *Appl. Opt.* **53**, 3508–3519 (2014)
 12. Bünger, L., Taubert, R. D., Anhalt, K.: Spectrally resolved radiometric characterisation and calibration using a supercontinuum laser in the NIR. In: *Proc. IRS²*, pp. 895–898 (2015)
 13. Marcet, S., Verhaegen, M., Blais-Ouellette, S., Martel, R.: Raman spectroscopy hyperspectral imager based on bragg tunable filter. *Proc. SPIE* **8231**, 82310U1–8 (2012)
 14. Gagnon, D., Dion-Bertrand, L.I.: Widely tunable filter technology and measurement of critical specifications. White Paper. Photon Etc., pp. 1–13 (2015)
 15. Photon Etc.: Laser Line Tunable Filter (LLTF) contrastTM. Instruction Manual, pp. 21–22 (2017)
 16. Vaskuri, A.: Multi-Wavelength setup based on lasers for characterizing optical detectors and materials. Master's Thesis, Aalto University (2014)
 17. Hamilton, C.A., Day, G.W., Phelan, R.J.: An electrically calibrated pyroelectric radiometer system. Technical Note 678, Electromagnetics Division Institute for Basic Standards, pp. 2–10. National Bureau of Standards, CO, USA (1976)
 18. Laser Probe Inc.: RKP-575 pyroelectric power probe: Datasheet, NY, USA
 19. Hamamatsu: Characteristics and use of infrared detectors. Technical Information, Hamamatsu Photonics K. K., Solid State Division, Japan (2011)
 20. Manoocheri, F., Kärhä, P., Palva, L., Toivanen, P., Haapalinnä, A., Ikonen, E.: Characterisation of optical detectors using high-accuracy instruments. *Anal. Chim. Acta.* **380**, 327–337 (1999)
 21. Eppeldauer, G.P.: Electronic characteristics of Ge and InGaAs radiometers. *Proc. SPIE* **3061**, 833–838 (1997)
 22. Stock, K.D.: Internal quantum efficiency of Ge photodiodes. *Appl. Opt.* **27**, 12–14 (1988)
 23. Lamminpää, A., Noorma, M., Hyypää, T., Manoocheri, F., Kärhä, P., Ikonen, E.: Characterization of germanium photodiodes and trap detector. *Meas. Sci. Technol.* **17**, 908–912 (2006)

Publisher's Note Springer Nature remains neutral with regard to jurisdictional claims in published maps and institutional affiliations.