
This is an electronic reprint of the original article.
This reprint may differ from the original in pagination and typographic detail.

Nefedova, Irina; Moradikouchi, Anis; Baggio, Mariangela; Tamminen, Aleksii; Hu, Yong; Ala-Laurinaho, Juha; Rodilla, Helena; Stake, Jan; Taylor, Zachary

Design of a quasioptical test bench for VNA extenders

Published in:

2020 45th International Conference on Infrared, Millimeter, and Terahertz Waves, IRMMW-THz 2020

DOI:

[10.1109/IRMMW-THz46771.2020.9370697](https://doi.org/10.1109/IRMMW-THz46771.2020.9370697)

Published: 08/11/2020

Document Version

Peer-reviewed accepted author manuscript, also known as Final accepted manuscript or Post-print

Please cite the original version:

Nefedova, I., Moradikouchi, A., Baggio, M., Tamminen, A., Hu, Y., Ala-Laurinaho, J., Rodilla, H., Stake, J., & Taylor, Z. (2020). Design of a quasioptical test bench for VNA extenders. In *2020 45th International Conference on Infrared, Millimeter, and Terahertz Waves, IRMMW-THz 2020* (pp. 552-553). Article 9370697 (International Conference on Infrared, Millimeter, and Terahertz Waves). IEEE. <https://doi.org/10.1109/IRMMW-THz46771.2020.9370697>

This material is protected by copyright and other intellectual property rights, and duplication or sale of all or part of any of the repository collections is not permitted, except that material may be duplicated by you for your research use or educational purposes in electronic or print form. You must obtain permission for any other use. Electronic or print copies may not be offered, whether for sale or otherwise to anyone who is not an authorised user.

Design of a quasioptical test bench for VNA extenders

Irina Nefedova¹, Anis Moradikouchi², Mariangela Baggio¹, Aleksi Tamminen¹, Yong Hu³, Juha Ala-Laurinaho¹, Helena Rodilla², Jan Stake³, Zachary Taylor¹
¹Aalto University, MilliLab, Espoo, Finland
²Chalmers University of Technology, Gothenburg, Sweden
³University of California, Los Angeles, USA

Abstract—The CAD design, simulated optical performance, and test measurements of a quasioptical test bench for VNA extenders are presented. The system allows straightforward integration of off axis parabolic mirrors and VNA extenders. The mirror orientation reduces aberrations and results suggest optical properties are close to what is expected with geometric ray tracing.

I. INTRODUCTION

THz imaging and spectroscopy applications often require close integration with collimating and focusing of THz radiation [1]. This optical instrumentation is commonplace for typical THz time-domain systems (TDS) but less reported on for vector-network analyzer (VNA) extender-based systems. This abstract reports on the design, simulation, fabrication, and testing of a quasioptical test bench for VNA extenders of various ranges.

coupled diode lasers for alignment assistance. Mirrors 1 and 4 (Fig. 2 Top) are coupled to the extenders, while mirrors 2 and 3 (Fig. 2: Bottom) focus/collect radiation to/from the target. All components are mounted on shared dovetail rails enabling rough adjustment and repeatable re-mounting.

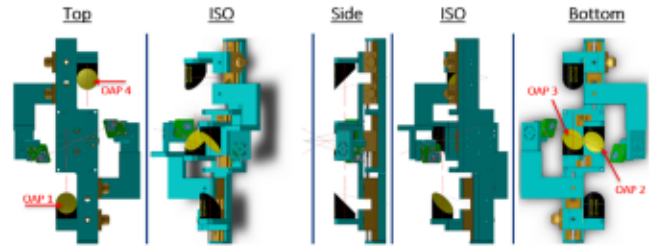


Fig. 2. CAD design of THz optics sub-assembly

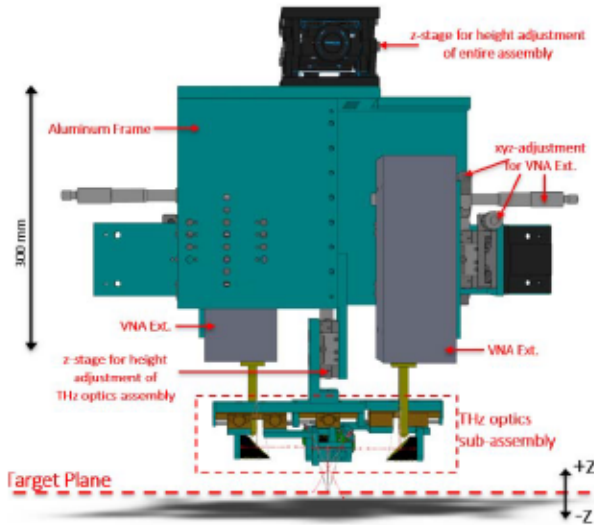


Fig. 1. CAD design of quasioptical system

A CAD drawing of the design is shown in Fig. 1. The main assembly consists of two VNA extenders labeled “VNA Ext.”. The THz optical system, labeled “THz optics sub-assembly” consists of four off-axis parabolic (OAP) mirrors to collimate, focus, and collect radiation to and from the target plane [2]. The assembly is indicated by the dashed rectangle in Fig. 1. The foci of the assembly are aligned with the extender feeds through a precision z-axis stage. The extenders are mounted in a downward facing orientation allowing the OAP mirror aperture edges to set the working distance between system and device under test (DUT).

Varying view angles of the THz optical system CAD design are shown in Fig. 2. The assembly is rotationally symmetric and consists of four 90° OAP mirrors and two kinematic mount

OAP Mirrors 2 and 3 can be swapped for matching pairs with varying focal lengths while keeping mirrors 1 and 4 and the overall optical assembly fixed. This enables on-target optical parameter exploration without re-alignment.

Fig. 3 shows the manufactured and constructed setup. The THz optics assembly was mounted on a rigid aluminum rail suspended above the optical table by 4 75 mm x 75 mm thick aluminum extrusions. Observation of metallic reflectors suggest minimum mirror and extender vibration.

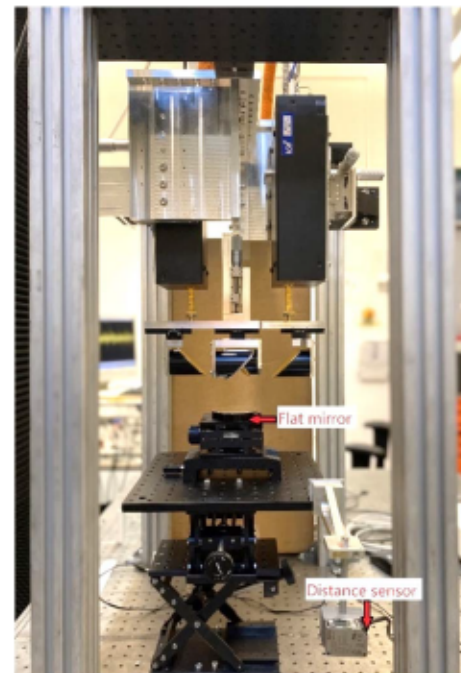


Fig. 3. Assembled quasioptical system with sample stage mounted below the OAP mirror train.

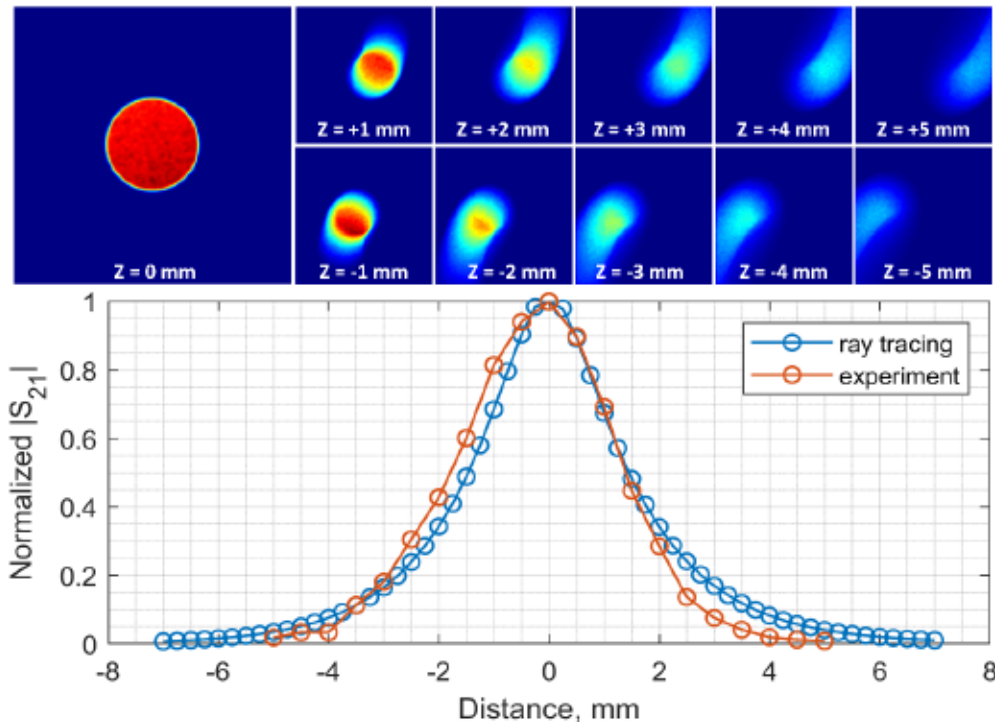


Fig. 4. Top: Ray-tracing results of target misalignment due to placement. Bottom: measured change in absolute value of S_{21} due to -5- and +5-mm displacement in z -plane.

II. RESULTS

Measurements of the system depth of focus were realized with a VNA (N522B PNA by Keysight Technologies) coupled to millimeter-wave extension modules (WR 2.2-VNAX by Virginia Diodes Ltd). The main limitation of the proposed design is inability to perform the traditional full two-port calibration. Standard SOLT (Short-Open-Load-Thru) or TRL (Thru-Reflect-Line) routines are not realizable, for example, due to impossibility to connect two ports together for the Thru step. One may go for calibration a transmitting port only, although the accuracy will be questionable. A flat mirror was placed at the target plane and its elevation relative to the focal point shared by mirrors 2 and 3 was varied with a vertical translation stage. Height perturbation was verified with a laser range finder (OD1-B100H50U25 by SICK Sensor Intelligence)

The target height was varied from 5 millimeter below the focal point (-5mm) to 5 mm above (+5mm) in increments of 0.5 mm. Complex S_{21} was acquired at every step and depth of focus was estimated via band integrated, total power.

The optical performance of the system was estimated with non-sequential ray tracing package ASAP (Breault Research Organization). An emitting disk of 1-mm semi-radius and 15° half-power angle was used as a Gaussian beam source representation and placed in the focal plane of OAP 1. The target was moved in and out of the image plane ($\pm z$ in Fig. 1) and the received rays monitored at the OAP 4 focal plane. A mask was applied to the ray tracing derived irradiance to mimic the effective aperture of the extender diagonal feedhorn

The aligned case ($z = 0$ mm) disk image is in the left side of Fig. 4 (Top) and shows a small gradient in field density from bottom to top, due to the inherent asymmetry introduced by

OAP mirrors. The misaligned cases demonstrate increasing coma as the DUT distance from $z = 0$ is increased. However, the coma is asymmetric, suggesting the mirror radial asymmetry has a significant effect on the optical performance.

The normalized integrated radiance limited by the mask aperture, as a function of target height, is superimposed on the experimental data in Fig. 4. The good agreement indicate that the submillimeter wave/THz frequency properties OAP mirror optical train can be estimated by ray tracing alone and suggest aberrations have been limited by OAP orientation.

III. SUMMARY

A quasioptical test bench for VNA extenders was presented. The design enables extender use in imaging and spectroscopy situations commonly explored with TDS instrumentation. Practical trial of presented setup has been demonstrated high measurement accuracy: the overall losses of the system, obtained by placing flat mirror on the target plane and measuring reflectivity through S_{21} , was -2dB.

REFERENCES

- [1] F. Goldsmith, *Quasioptical Systems*, New York: IEEE Press, 1998.
- [2] S. Sung, J. Garritano, N. Bajwa, B. Nowroozi, W. Grundfest, and Z. Taylor, "Analysis and optimization of THz imaging optics with off-axis parabolic mirrors," *International Conference on Infrared, Millimeter, and Terahertz Waves, IRMMW-THz*, 11/13, 2014.