
This is an electronic reprint of the original article.
This reprint may differ from the original in pagination and typographic detail.

Lamberg, Joel; Zarrinkhat, Faezeh; Tamminen, Aleks; Khaled, Elsayed E.M.; Taylor, Zachary
Investigation of radial top-hat electric field distributions for corneal reflectometry using modified Fourier optics method

Published in:
2021 46th International Conference on Infrared, Millimeter, and Terahertz Waves, IRMMW-THz 2021

DOI:
[10.1109/IRMMW-THz50926.2021.9566964](https://doi.org/10.1109/IRMMW-THz50926.2021.9566964)

Published: 01/01/2021

Document Version
Peer-reviewed accepted author manuscript, also known as Final accepted manuscript or Post-print

Please cite the original version:
Lamberg, J., Zarrinkhat, F., Tamminen, A., Khaled, E. E. M., & Taylor, Z. (2021). Investigation of radial top-hat electric field distributions for corneal reflectometry using modified Fourier optics method. In *2021 46th International Conference on Infrared, Millimeter, and Terahertz Waves, IRMMW-THz 2021* (International Conference on Infrared, Millimeter, and Terahertz Waves). IEEE. <https://doi.org/10.1109/IRMMW-THz50926.2021.9566964>

This material is protected by copyright and other intellectual property rights, and duplication or sale of all or part of any of the repository collections is not permitted, except that material may be duplicated by you for your research use or educational purposes in electronic or print form. You must obtain permission for any other use. Electronic or print copies may not be offered, whether for sale or otherwise to anyone who is not an authorised user.

Investigation of radial top-hat electric field distributions for corneal reflectometry using modified Fourier optics method

Joel Lamberg¹, Faezeh Zarrinkhat^{1,2}, Aleksi Tamminen¹, Elsayed E. M. Khaled^{3,4}, Zachary Taylor¹

¹Department of Electronics and Nanoengineering, Aalto University, MilliLab, Espoo, Finland

²Technical University of Catalonia/UPC, Barcelona, Spain

³Department of Electrical Engineering, Assiut University, Assiut, Egypt

⁴High Institute for Engineering & Technology, Sohag, Egypt

Abstract—An efficient Fourier optics method for synthesizing a required incident beam to compute the internal and scattered electromagnetic fields from known spherical surface electric field distribution is presented.

I. INTRODUCTION

CONVENTIONAL methods for evaluating electromagnetic beams created from known spherical electric-field surface distributions may include full-wave simulations, geometric optics (GO), or physical optics (PO). These methods are extensively studied and accurate given the model fidelity and a suitable wavelength range. However, they cannot assess the internal and scattered electric fields on the multi-layered spherical objects without considerable computational effort and complexity.

Fourier optics is a powerful method to model an incident electric field that addresses the above-mentioned challenges [1]. For spherical targets, the field can be easily expanded via vector spherical harmonics (VSH) presentation to accommodate the geometry. The VSH presentation is mapped with the T-matrix method to evaluate internal and scattered fields from multi-layered dielectric spheres [2]. Nevertheless, this method is nominally limited to sources defined on a plane.

In this study, the Fourier optics method is expanded to model beam propagation from arbitrary electric field distributions positioned on spherical surfaces. The method's main idea is that Riemann's surface integral combines differential surface elements, which can be approximated as locally planar elements. The Fourier optics method is applied to each of these elements, and the total electric field is the sum of the fields created from them by the superposition principles [3].

The method is readily applicable to the field of THz sensing of corneal tissue hydration and geometry due to the cornea's layered spherical shell nature [4]. The derived formula for the incident electric field of the beam from a spherical surface distribution with differential elements is:

$$\mathbf{E}_{inc}(\mathbf{r}) = \frac{1}{4\pi^2} \iint_{\Omega} E_0(\theta, \varphi) \sin\theta \mathbf{E}_t(k\mathbf{r}; \theta, \varphi) d\theta d\varphi, \quad (1)$$

where $E_0(\theta, \varphi)$ is the complex surface amplitude, $k = 2\pi/\lambda$ is the wavenumber, and r, θ, φ are the spherical coordinates and $\mathbf{r} = r\mathbf{e}_r$ and \mathbf{e}_r is a radial unit-vector. Moreover, the electromagnetic beam from a differential source element with realistic polarization in (1) is presented with VSH as:

$$\mathbf{E}_t(k\mathbf{r}; \theta, \varphi) = p^2 \sum_m \sum_n D_{mn} [a_{emn}^t M_{emn}^1 + a_{omn}^t M_{omn}^1 + b_{emn}^t \mathbf{N}_{emn}^1 + b_{omn}^t \mathbf{N}_{omn}^1], \quad (2)$$

where p is a computational factor given in [2], D_{mn} is the normalization factor, $a_{emn}^t, a_{omn}^t, b_{emn}^t$ and b_{omn}^t are the

VSH coefficients, $M_{emn}^1, M_{omn}^1, N_{emn}^1$ and N_{omn}^1 are the VSH of the first kind [5].

II. RESULTS

The electric field with radial Gaussian and top-hat distributions was created on a spherical surface and simulated with MATLAB. The incident beam which makes such field distributions are obtained with the developed modified Fourier optics method. The optical axis of the incident beam is along the x-axis, and the beam is evaluated at the transverse zy - plane at 40 mm from the origin of the sphere (see Figure 1). The results are shown in Figures 3 – 4.

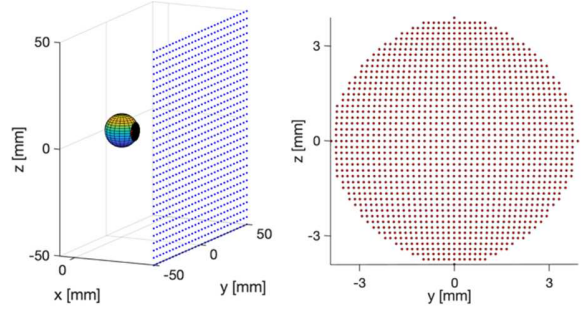


Fig. 1 The simulation arrangement, where red dots represent the source element locations and blue dots represent the evaluating plane.

The results of top-hat simulations are compared to identical PO simulations, and they are with a precise match down to -41 dB difference in amplitude and difference less than 0.32 degrees (average difference is 0.27 degrees) in phase at 275 GHz for the spherical surface with radius of curvature (RoC) of 7.8 mm that coincident with the beam curvature.

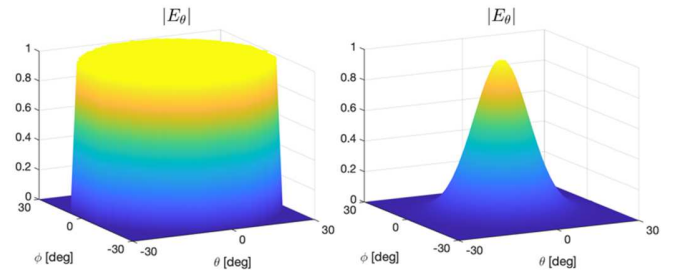


Fig. 2 The projected electric field distributions located at the spherical surface.

A comparison simulation was made with a Gaussian distribution at the sphere's surface. This beam is not a well-known Gaussian beam from a planar distribution, as the wave-front of the incident beam is synthesized from the equal phase spherical Gaussian distribution to match the cornea's surface.

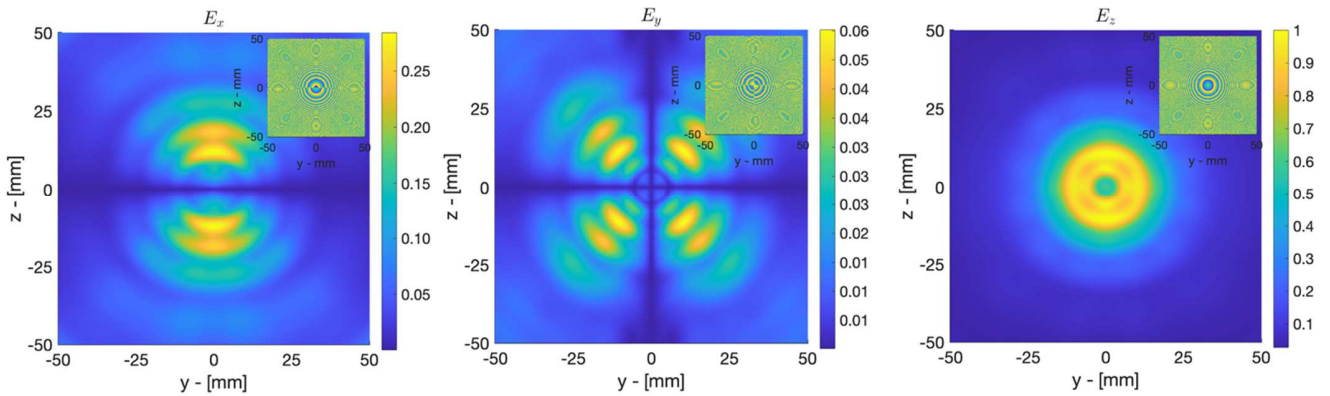


Fig. 3 The electric field components from the top-hat distribution at the zy -plane at 40 mm from the origin of the sphere, normalized by the main polarization \mathbf{E}_z .

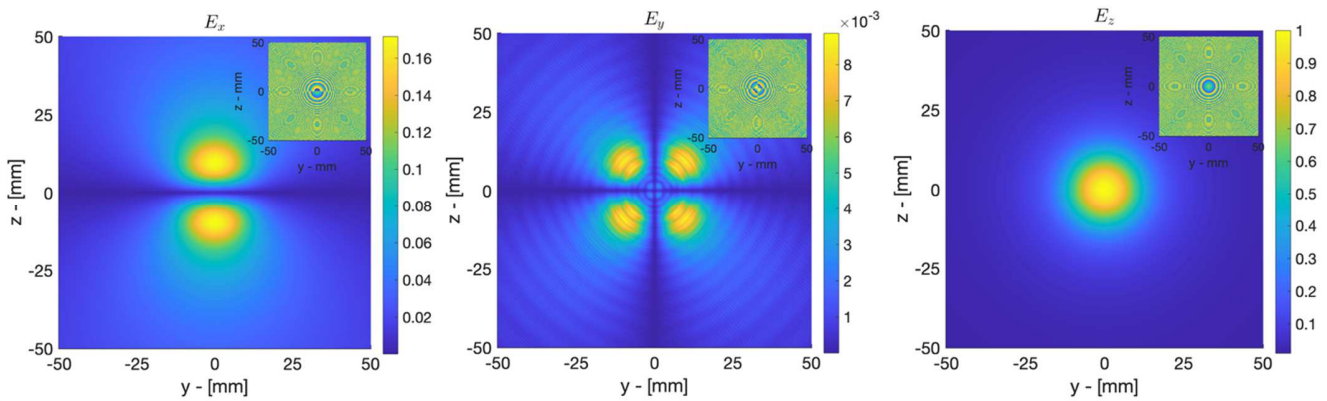


Fig. 4 The electric field components from the Gaussian distribution at the zy -plane at 40 mm from the origin of the sphere, normalized by the main polarization \mathbf{E}_z .

Figures 3 and 4 illustrate the required electric field components at a plane aperture for creating the incident beam with a spherical top-hat or Gaussian electric field distribution at the cornea's surface with the matching wavefront.

III. SUMMARY

The presented modified Fourier optics method was compared to numerous arrangements with known analytical methods or PO simulation results. Each comparison demonstrates good agreement combined with the novel ability to evaluate the internal and scattered fields from the multi-layered sphere. With this proposed method, the complex electric field distribution at the spherical surface can be discretized and distributed arbitrarily. If the phase is uniform and fixed at each discretization point, the incident beam's wavefront matches the spherical surface across the illuminated area. This feature of wavefront matching enables analysis with standard Fresnel equations and stratified medium theory.

The minimum wavelength of the electric field to simulate an incident beam from the spherical surface is approximately $RoC \geq 2\lambda$, due to the nature of the Fourier-optics. When RoC is below the limit, the simulation error increases faster with the total phase and at the periphery of the surface. The vector spherical harmonic presentation, on the other hand, creates a computational upper limit for the frequency. Thus, more VHS modes are needed to compute the presented results at higher frequencies for a given RoC . For this reason, the presented

method is optimal for simulating the electromagnetic behavior of the cornea with THz frequencies due to the size parameter range defined by the band of interest and the corneal RoC .

REFERENCES

- [1] Joseph W. Goodman, *Introduction to Fourier optics*, 3rd edition, Englewood, CO: Roberts, 2005.
- [2] E. E. M. Khaled, S. C. Hill, and P. W. Barber, "Scattered and internal intensity of a sphere illuminated with a Gaussian beam," *IEEE Transactions on Antennas and Propagation*, vol. 41, pp. 295-303, 1993.
- [3] S.C. Hill and P.W. Barber, *Light Scattering By Particles: Computational Methods*, Advanced Series in Applied Physics, 1990.
- [4] Z. D. Taylor *et al.*, "THz and mm-Wave Sensing of Corneal Tissue Water Content: Electromagnetic Modeling and Analysis," in *IEEE Transactions on Terahertz Science and Technology*, vol. 5, no. 2, pp. 170-183, March 2015, doi: 10.1109/TTHZ.2015.2392619.
- [5] C. Bohren and D. R. Huffman, *Absorption and Scattering of Light by Small Particles*. Wiley Science Paperback Series, 1998.